



UPSTATE

MEDICAL UNIVERSITY

Materials Management


Clinical Supplies, Materials and Logistics



Foley Catheter Insertion Tray (Lawson #54445):

Problem:

- Bard Foley catheter insertion trays are on long term backorder.
- Trays made by Covidien/Medline are being substituted.
- The Covidien/Medline substitute trays DO NOT CONTAIN POVIDONE IODINE SWABS.

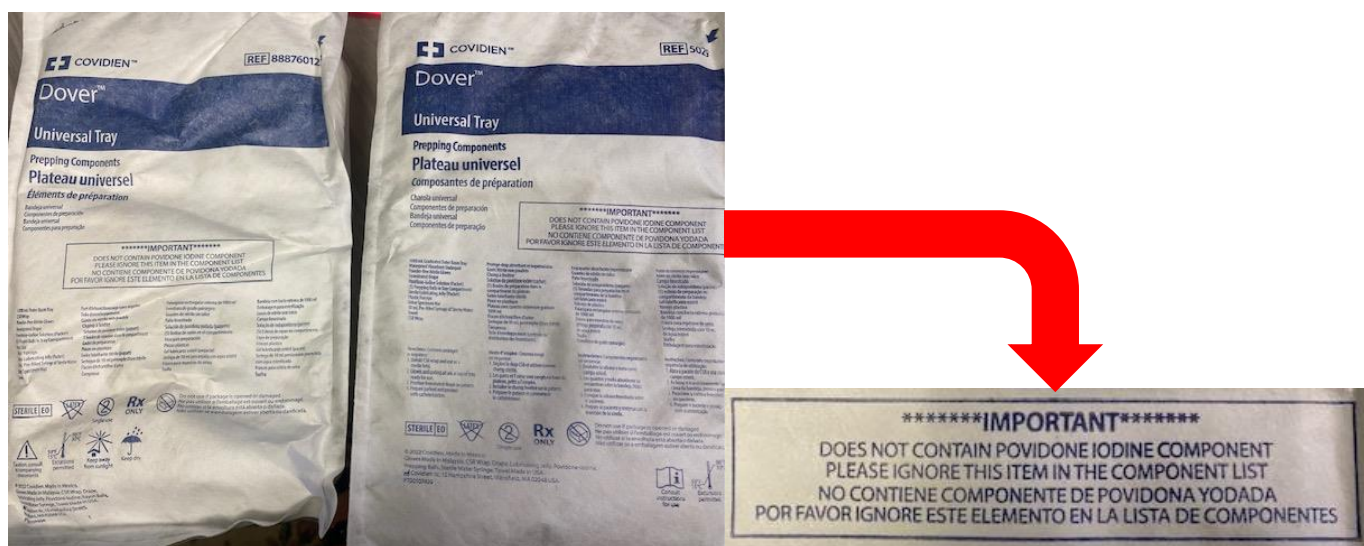

Action:

- Verify that the sub tray has a notice stating it is missing the povidone iodine swabs.
- Obtain povidone iodine swabs separately prior to using tray.