



70 um 70 psi Aria III upgrade

Cytometer:	FACSAriaII	User:	Administrator
Cytometer Name:	FACSAriaII	Institution:	
Serial Number:	1	Software:	BD FACSDiva 6.1.2
Input Device:	Manual	Date:	10/22/2013 12:22:31 PM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


Red Laser (633nm)

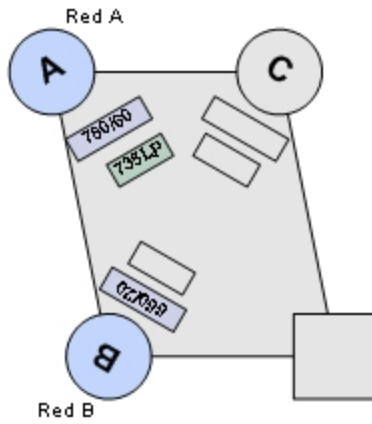


Blue Laser (488nm)

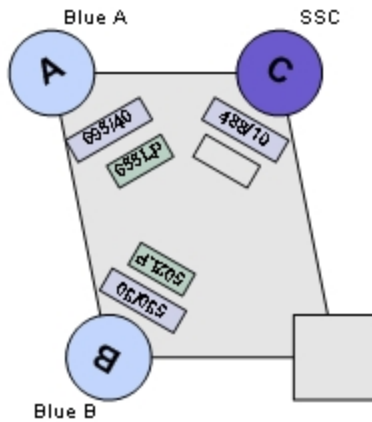

Violet Laser
(407nm)

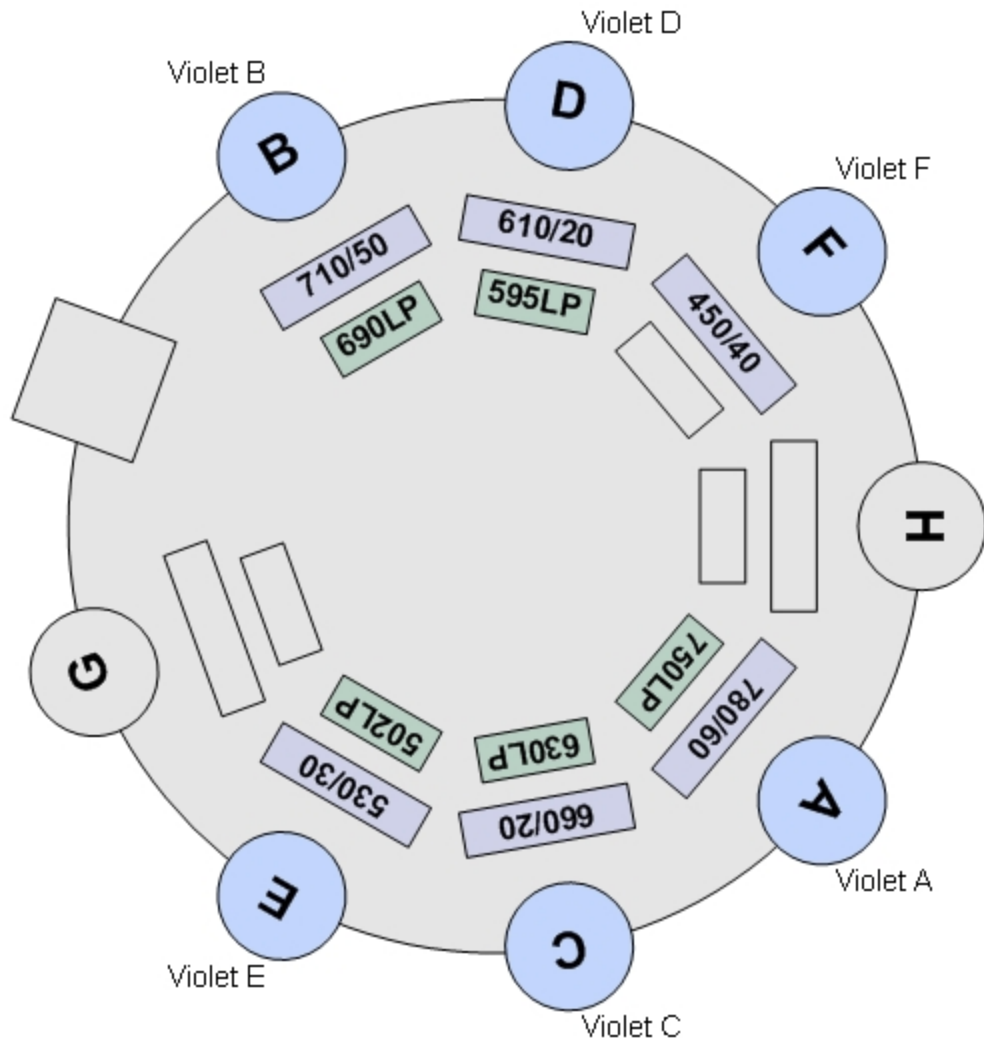

Yellow Green Laser
(561nm)

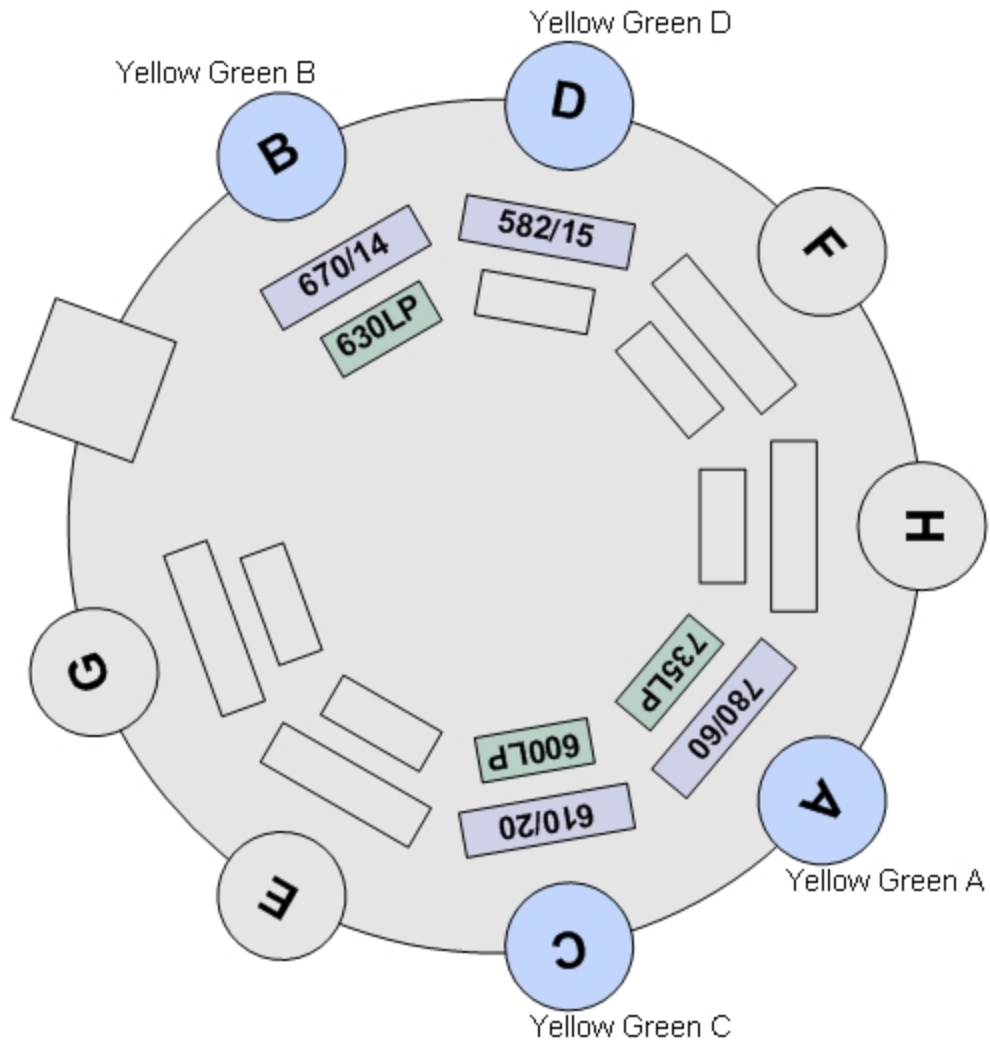

Comments: